



ABN 43 064 478 842

➤ 231 osborne avenue clayton south, vic 3169
PO box 1548, clayton south, vic 3169
t 03 9265 7400 f 03 9558 0875
freecall 1800 680 680
www.tmgtestequipment.com.au

Test & Measurement

- sales
- rentals
- calibration
- repair
- disposal

Complimentary Reference Material

This PDF has been made available as a complimentary service for you to assist in evaluating this model for your testing requirements.

TMG offers a wide range of test equipment solutions, from renting short to long term, buying refurbished and purchasing new. Financing options, such as Financial Rental, and Leasing are also available on application.

TMG will assist if you are unsure whether this model will suit your requirements.

Call TMG if you need to organise repair and/or calibrate your unit.

If you click on the "Click-to-Call" logo below, you can call us for FREE!

TMG Corporate Website

TMG Products Website



Click-to-Call
TMG Now



Disclaimer:

All trademarks appearing within this PDF are trademarks of their respective owners.



Instructions



P6150

For 50 Ohm Oscilloscopes

070-7173-01

Warning

The servicing instructions are for use by qualified personnel only. To avoid personal injury, do not perform any servicing unless you are qualified to do so. Refer to all safety summaries prior to performing service.

Copyright © Tektronix, Inc. All rights reserved.

Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supercedes that in all previously published material. Specifications and price change privileges reserved.

Printed in the U.S.A.

Tektronix, Inc., P.O. Box 1000, Wilsonville, OR 97070-1000

TEKTRONIX and TEK are registered trademarks of Tektronix, Inc.

WARRANTY

Tektronix warrants that the products that it manufactures and sells will be free from defects in materials and workmanship for a period of one (1) year from the date of purchase from an authorized Tektronix distributor. If any such product proves defective during this warranty period, Tektronix, at its option, either will repair the defective product without charge for parts and labor, or will provide a replacement in exchange for the defective product. Batteries are excluded from this warranty.

In order to obtain service under this warranty, Customer must notify Tektronix of the defect before the expiration of the warranty period and make suitable arrangements for the performance of service. Customer shall be responsible for packaging and shipping the defective product to the service center designated by Tektronix, shipping charges prepaid, and with a copy of customer proof of purchase. Tektronix shall pay for the return of the product to Customer if the shipment is to a location within the country in which the Tektronix service center is located. Customer shall be responsible for paying all shipping charges, duties, taxes, and any other charges for products returned to any other locations.

This warranty shall not apply to any defect, failure or damage caused by improper use or improper or inadequate maintenance and care. Tektronix shall not be obligated to furnish service under this warranty a) to repair damage resulting from attempts by personnel other than Tektronix representatives to install, repair or service the product; b) to repair damage resulting from improper use or connection to incompatible equipment; c) to repair any damage or malfunction caused by the use of non-Tektronix supplies; or d) to service a product that has been modified or integrated with other products when the effect of such modification or integration increases the time or difficulty of servicing the product.

THIS WARRANTY IS GIVEN BY TEKTRONIX WITH RESPECT TO THE LISTED PRODUCTS IN LIEU OF ANY OTHER WARRANTIES, EXPRESS OR IMPLIED. TEKTRONIX AND ITS VENDORS DISCLAIM ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. TEKTRONIX' RESPONSIBILITY TO REPAIR OR REPLACE DEFECTIVE PRODUCTS IS THE SOLE AND EXCLUSIVE REMEDY PROVIDED TO THE CUSTOMER FOR BREACH OF THIS WARRANTY. TEKTRONIX AND ITS VENDORS WILL NOT BE LIABLE FOR ANY INDIRECT, SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES IRRESPECTIVE OF WHETHER TEKTRONIX OR THE VENDOR HAS ADVANCE NOTICE OF THE POSSIBILITY OF SUCH DAMAGES.

Contacting Tektronix

Product Support

For application-oriented questions about a Tektronix measurement product, call toll free in North America:

1-800-TEK-WIDE (1-800-835-9433 ext. 2440)

6:00 a.m. – 5:00 p.m. Pacific time

Or contact us by e-mail:

tm_app_supp@tek.com

For product support outside of North America, contact your local Tektronix distributor or sales office.

Service Support

Contact your local Tektronix distributor or sales office. Or visit our web site for a listing of worldwide service locations.

<http://www.tek.com>

For other information

In North America:

1-800-TEK-WIDE (1-800-835-9433)

An operator will direct your call.

To write us

Tektronix, Inc.

P.O. Box 1000

Wilsonville, OR 97070-1000

General Safety Summary

Review the following safety precautions to avoid injury and prevent damage to this product or any products connected to it. To avoid potential hazards, use this product only as specified.

To Avoid Fire or Personal Injury

Connect and Disconnect Properly. Do not connect or disconnect probes or test leads while they are connected to a voltage source.

Observe All Terminal Ratings. To avoid fire or shock hazard, observe all ratings and markings on the product. Consult the product manual for further ratings information before making connections to the product.

The common terminal is at ground potential. Do not connect the common terminal to elevated voltages.

Do not apply a potential to any terminal, including the common terminal, that exceeds the maximum rating of that terminal.

Do Not Operate With Suspected Failures. If you suspect there is damage to this product, have it inspected by qualified service personnel.

Do Not Operate in Wet/Damp Conditions.

Do Not Operate in an Explosive Atmosphere.

Keep Product Surfaces Clean and Dry.

Symbols and Terms



Terms in this Manual. These terms may appear in this manual:

CAUTION. *Caution statements identify conditions or practices that could result in damage to this product or other property.*

Operating Basics

The P6150 is a high-frequency low-capacitance passive probe designed to be used with 11800 Series oscilloscopes. The P6150 comes standard with a one meter SMA male-to-male cable assembly and 1X and 10X attenuators. The probe head has a female SMA connector that screws into the cable assembly.

The low capacitance and constant input resistance of the P6150 make it possible to probe high-frequency circuits without disturbing the circuit with a large capacitive load.

This manual describes the operation of the P6150 probe connected to a Tektronix 11801/11802 sampling oscilloscope with SD-24/SD-26 sampling head. The P6150 probe may also be used with any 50 Ω input instrumentation.



CAUTION. Before connecting the probe to the SD-24 sampling head, you should eliminate potential electrostatic build up from the probe cable. To discharge the cable with the probe head attached, momentarily connect the probe tip to the cable or probe ground. A charge stored in the 50 Ω cable (if at high enough voltage) can damage the SD-24 input.

To maintain consistent signal quality, torque system SMA connectors to 5 inch-pounds.

Do not exceed the input voltage rating of the sampling head (± 3 V for SD-24) or damage to the head can result. The peak input voltage rating is increased by the attenuation factor of the probe head (for example, 10X times ± 3 V is ± 30 V).

The RMS input voltage rating is limited by the power handling capacity of the attenuator resistor. For example, if the 10X attenuator is rated at 1/4 watt, the RMS input voltage should be limited to less than 12.5 V_{RMS}.

The ceramic probe tip resistor network in the 10X probe head is very susceptible to damage if excessive vertical or angular pressure is applied.



CAUTION. The ceramic resistor network is in danger of breaking if more than five pounds of vertical (down) pressure or more than three pounds of angular pressure (pressure that will cause the resistor to attempt to flex), is applied to the probe tip or ceramic resistor.

Avoid excessive vertical or angular pressure, dropping or hitting the probe, or allowing the probe to swing against a hard surface. Always place the probe-tip protector (supplied) on the tip when the probe is not in use.

System Response

Figure 1 shows typical system responses with various cable and attenuator combinations. The system consists of a Tektronix 11801 sampling oscilloscope and SD-24 TDR sampling head driven by the internal calibrator pulser.

1. Response of 22 cm cable (174-1120-00); 50 mV/div, $t_r = 30$ ps.
2. Response of 1 m cable (174-1341-00); 50 mV/div, $t_r = 43$ ps.
3. Response of 1 m cable with the 10X probe head in the probe tip adapter. (013-0251-00); 5 mV/div, $t_r = 39$ ps.
4. Response of the 10X probe head with 22 cm cable (174-1120-00); 5 mV/div, $t_r = 32$ ps.

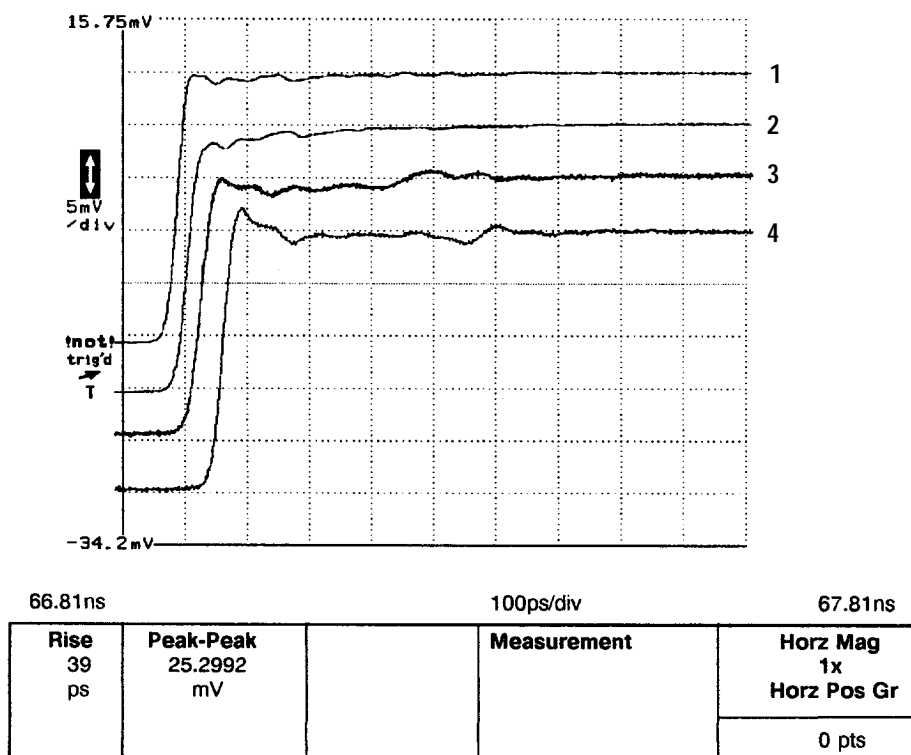


Figure 1: Typical system response

Probe Tip Grounding

The quality of ground at the probe tip affects performance. For minimum rise time and aberrations, keep the ground lead short and the ground contact as close as possible to the point being probed.

Figure 3 shows typical system responses with different probe tip grounding methods. Measurements were taken with the 10X attenuator head while probing the microstrip line on the probe tip adapter (013-0251-00).

1. Response with 013-0251-00 probe tip adapter, $t_r = 38$ ps.
2. Response with ground clip cut to the probe tip length. (package of 20 included with accessories: 020-1708-00; $t_r = 52$ ps.
3. Response with full length ground clip. (package of 20 included with accessories: 020-1708-00); $t_r = 81$ ps.

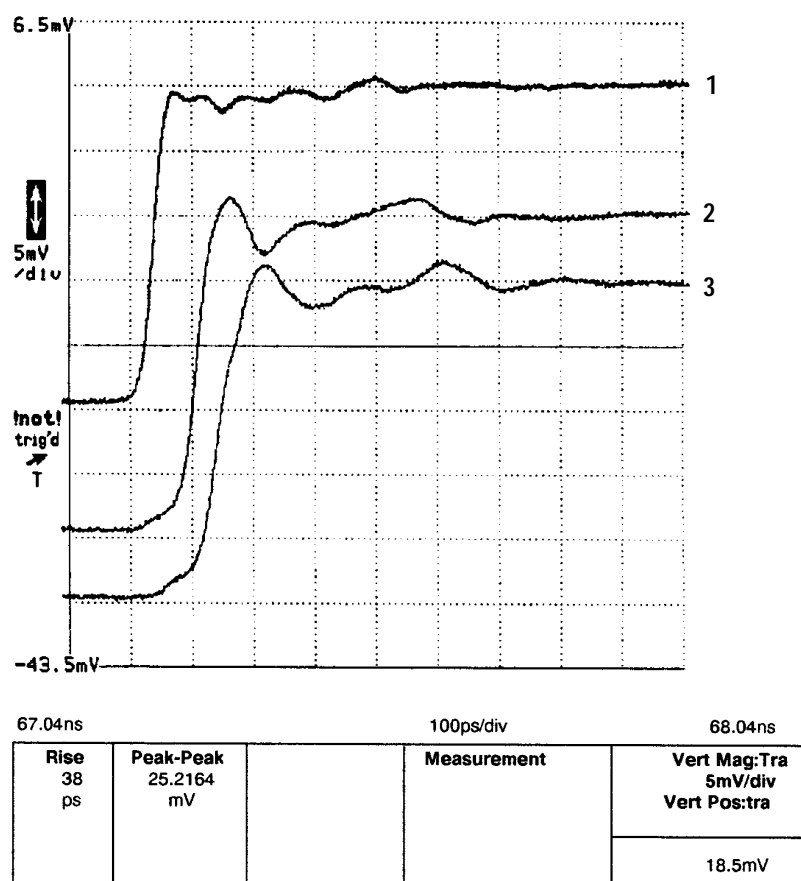


Figure 2: Probe tip grounding

Input Impedance

Typical input impedance vs frequency of the 10X attenuator.

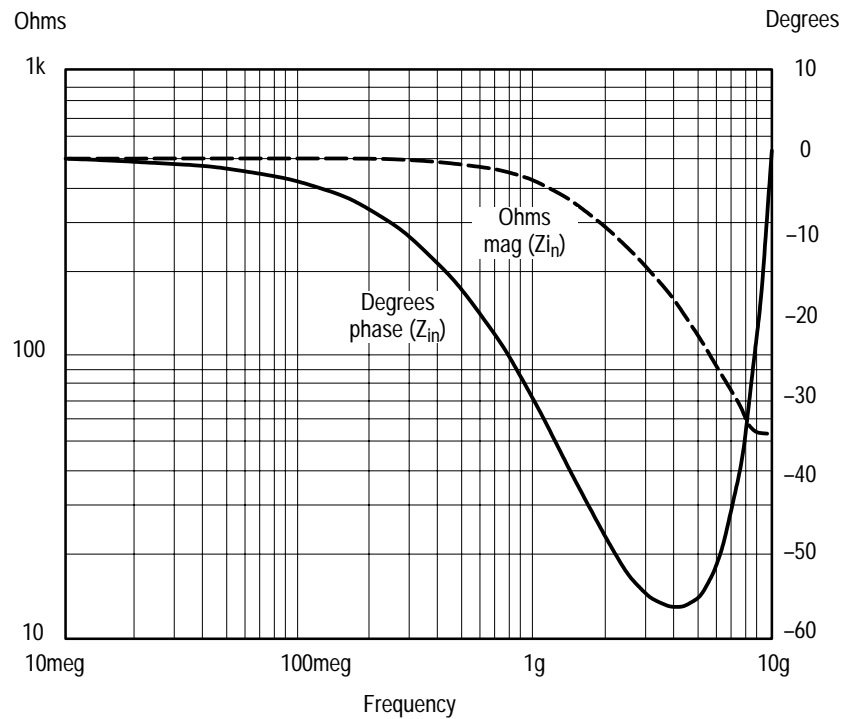


Figure 3: Input impedance

Attenuator Color Coding

Table 1 identifies P6150 probe tip attenuation factors by color color coding.

Table 1: Probe tip attenuation factors

Color	Attenuation Factor
Black	1X
Blue	10X

Maintenance

Use the following procedures to clean and maintain the P6150 probe.

Cleaning

Remove accumulated dust from the outside of the probe with a soft cloth or a small brush. Remove any remaining dirt with a soft cloth dampened in a mild detergent and water solution. Do not use abrasive cleaners.



CAUTION. Do not use cleaning agents that may damage the plastic components of the probe. In particular, avoid solvents such as benzene, toluene, xylene, acetone, or MEK.

Probe Module Replacement

The P6150 probe heads are sealed and contain no user-serviceable parts.

Specifications

The following specifications apply when the instrument warms up for a period of at least 20 minutes in an environment that does not exceed the limits described in Table 3 below.

Table 2: Electrical characteristics

Characteristic	1X	10X
Attenuation Tolerance ^{1,2}	±2%	±2%
Input Resistance ¹	50 Ω +2% -1%	500 Ω ±1.25%
Input Capacitance	N/A	≤0.15 pF
Maximum Continuous Nondestructive Input Voltage	Oscilloscope maximum input voltage	12.5 V _{RMS}
Bandwidth at Probe Tip ³	≥3.0 GHz	9 GHz
Rise Time at Probe Tip ³	≤170 ps	≤38.8 ps
Signal Delay	4.40 ±0.1 ns	4.40 ±0.1 ns

¹ System characteristic.

² Oscilloscope input must be 50 Ω ±1%.

³ In-system measurement.

Table 3: Environmental characteristics

Characteristic	Description
Temperature Range	
Operating	-15° C to +55° C (+5° F to +131° F)
Nonoperating	-62° C to +85° C (-80° F to +185° F)
Humidity ¹	Five cycles (120 hr) at 95% to 97% relative humidity 30° C to 60° C

¹ Reference to MIL-E-1600F, paragraph 4.5.9 through 4.5.9.5.1, class 4.

Table 4: Physical characteristics

Characteristic	Description
Length	1 m (3.3 ft.)
Shipping Weight	595 g (1.31 lbs.)

Replaceable Parts

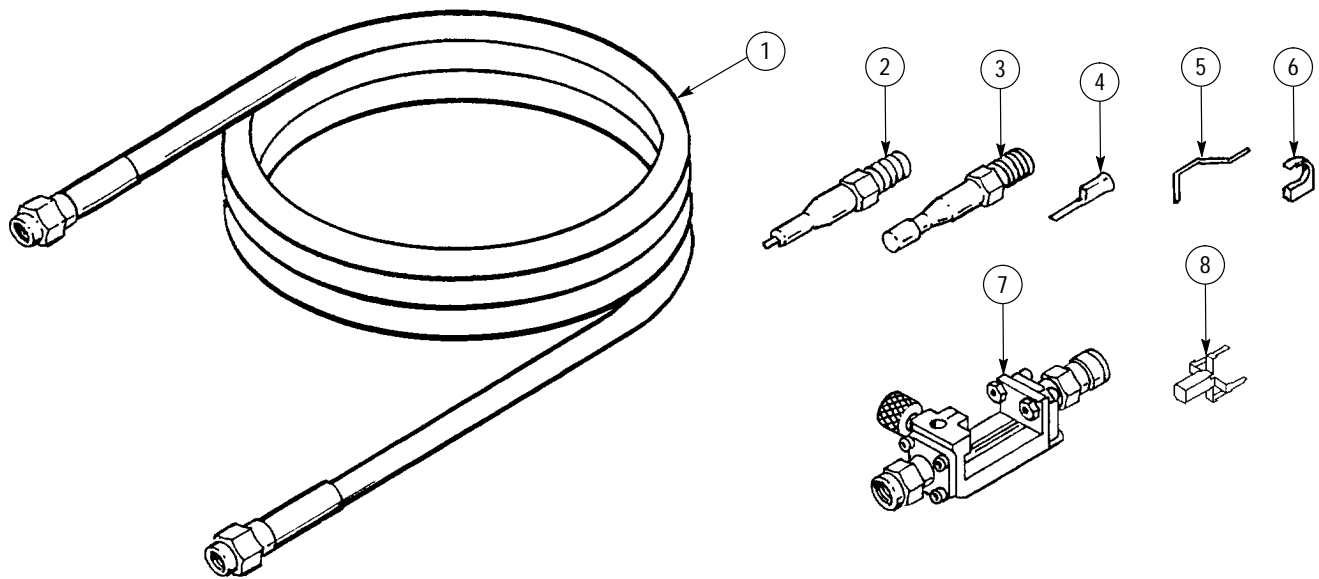


Figure 4: P6150 probe with accessories

Replaceable parts: P6150 probe and accessories

Fig. & index number	Tektronix part number	Serial no. effective	Serial no. discont'd	Qty	Name & description	Mfr. code	Mfr. part number
P6150							
4 -1	174-1341-00			1	CABLE ASSY,RF:50 OHM COAX,39.37 L,8-N	60381	500-1117-00
-2	206-0398-00			1	PROBE HEAD ASSY:1X P6150	80009	206-0398-00
-3	206-0399-00		8905	2	PROBE HEAD ASSY:10X,RES NTWK,450 OHM	80009	206-0399-00
	206-0399-02	8906		2	PROBE HEAD ASSY:10X RES NTWK,450 OHM	80009	206-0399-02
STANDARD ACCESSORIES							
	020-1708-00			1	ACCESSORY PKG:STANDARD ACCESS TO P6150	80009	020-1708-00
-4	-----			20	.CONTACT,ELEC:GND,CLIP,PH,BRZ (ORDER 020-1708-00)		
-5	-----			10	.CONTACT,ELEC:GND,LEAD,0.025 WIRE NICKEL (ORDER 020-1708-00)		
-6	-----			3	.CONTACT,ELEC:0.025 NICKEL ALLOY 52 WIRE (ORDER 020-1708-00)		
	070-7173-00			1	SHEET,TECHNICAL:P6150	TK2548	PER TEK P/N
	174-1341-00			1	CABLE ASSY,RF:50 OHM COAX,39.37 L,8-N	60381	500-1117-00
OPTIONAL ACCESSORIES							
	174-1120-00			1	CA ASSY,RF:COAXIAL,RFD,50 OHM,8.5 L	TK2469	174-1120-00
	206-0398-00			1	PROBE HEAD ASSY:1X	80009	206-0398-00
	206-0398-01		8904	1	PROBE HEAD ASSY:PKG OF 5,1X	80009	206-0398-01
	206-0399-00		8904	1	PROBE HEAD ASSY:10X,RES NTWK,450 OHM	80009	206-0399-00
	206-0399-01		8904	1	PROBE HEAD ASSY:PKG OF 3,10X	80009	206-0399-01
	206-0399-02	8905		1	PROBE HEAD ASSY:10X	80009	206-0399-02
-7	013-0251-00			1	ADAPTER,P TIP:SMA TO P6150	80009	013-0251-00
-8	131-4209-00			1	CONNECTOR,PROBE:PROBE TO CKT BD ADAPTER	80009	131-4209-00

Manufacturers cross index

Mfr. code	Manufacturer	Address	City, state, zip code
60381	PRECISION INTERCONNECT CORP.	16640 SW 72ND AVE	PORTLAND, OR 97224
80009	TEKTRONIX INC	14150 SW KARL BRAUN DR PO BOX 500	BEAVERTON, OR 97077-0001
TK2469	UNITREK CORPORATION	3000 LEWIS & CLARK HWY SUITE 2	VANCOUVER, WA 98661