

ABN 43 064 478 842

231 osborne avenue clayton south, vic 3169
PO box 1548, clayton south, vic 3169
t 03 9265 7400 f 03 9558 0875
freecall 1800 680 680
www.tmgtestequipment.com.au

### Test & Measurement

### **Complimentary Reference Material**

sales
rentals
calibration
repair
disposal
This PDF has been made available as a complimentary service for you to assist in evaluating this model for your testing requirements.
TMG offers a wide range of test equipment solutions, from renting short to long term, buying refurbished and purchasing new. Financing options, such as Financial Rental, and Leasing are also available on application.
TMG will assist if you are unsure whether this model will suit your requirements.
Call TMG if you need to organise repair and/or calibrate your unit.
If you click on the "Click-to-Call" logo below, you can all us for FREE!



#### **Disclaimer:**

All trademarks appearing within this PDF are trademarks of their respective owners.



Instructions

# Tektronix

# 012-1568-00 and 012-1569-00 80E00 Series Sampling Module Extenders

071-0436-01

www.tektronix.com

071043601

Copyright © Tektronix, Inc. All rights reserved.

Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supercedes that in all previously published material. Specifications and price change privileges reserved.

Tektronix, Inc., P.O. Box 500, Beaverton, OR 97077

TEKTRONIX and TEK are registered trademarks of Tektronix, Inc.

#### WARRANTY

Tektronix warrants that the parts, assemblies and supplies ("products") that it manufactures and sells will be free from defects in materials and workmanship for a period of three (3) months from the date of shipment. If a product proves defective during this warranty period, Tektronix, at its option, either will repair the defective product without charge for parts and labor, or will provide a replacement in exchange for the defective product.

In order to obtain service under this warranty, Customer must notify Tektronix of the defect before the expiration of the warranty period and make suitable arrangements for the performance of service. Customer shall be responsible for packaging and shipping the defective product to the service center designated by Tektronix, with shipping charges prepaid. Tektronix shall pay for the return of the product to Customer if the shipment is to a location within the country in which the Tektronix service center is located. Customer shall be responsible for paying all shipping charges, duties, taxes, and any other charges for products returned to any other locations.


This warranty shall not apply to any defect, failure or damage caused by improper use or improper or inadequate maintenance and care. Tektronix shall not be obligated to furnish service under this warranty a) to repair damage resulting from attempts by personnel other than Tektronix representatives to install, repair or service the product; b) to repair damage resulting from improper use or connection to incompatible equipment; c) to repair any damage or malfunction caused by the use of non-Tektronix supplies; or d) to service a product that has been modified or integrated with other products when the effect of such modification or integration increases the time or difficulty of servicing the product.

THIS WARRANTY IS GIVEN BY TEKTRONIX IN LIEU OF ANY OTHER WARRANTIES, EXPRESS OR IMPLIED. TEKTRONIX AND ITS VENDORS DISCLAIM ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE. TEKTRONIX' RESPONSIBILITY TO REPAIR OR REPLACE DEFECTIVE PRODUCTS IS THE SOLE AND EXCLUSIVE REMEDY PROVIDED TO THE CUSTOMER FOR BREACH OF THIS WARRANTY. TEKTRONIX AND ITS VENDORS WILL NOT BE LIABLE FOR ANY INDIRECT, SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES IRRESPECTIVE OF WHETHER TEKTRONIX OR THE VENDOR HAS ADVANCE NOTICE OF THE POSSIBILITY OF SUCH DAMAGES.

## **Product Description**

The Sampling Module Extender can be used to extend the reach of any 80E00 Series Sampling Module from the instrument in which it is installed. The extender is intended for use with the CSA8000 Communications Signal Analyzer or the TDS8000 Digital Sampling Oscilloscope. The extender is installed between the sampling module and the instrument, allowing the sampling module to be operated out of the module compartment in the instrument.

The term "extender" refers to either of the following two extenders, available in two lengths:

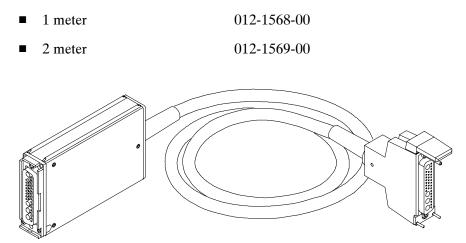

### Why Use?

Use the extender to extend the sampling module out of its instrument compartment to reach the device under test. Using the extender avoids input-signal degradation that can occur when using interconnect cables between the sampling module and the device under test to extend reach.

### **Exclusions**

Observe the following usage rules to avoid damaging your sampling modules or instruments:

- The extender can be used only with electrical sampling modules (80E00 series); it is not usable with optical modules (80C00 series).
- The extender can only be used with the CSA8000 or the TDS8000 instrument and its sampling modules; do NOT attempt to use this extender with an

11800 or a CSA800 series instrument. Instead, use the extender made solely for the 11800 and the CSA800 instrument.

Also, do not attempt to use the extender cable that was made solely for the 11800 and CSA800 instrument with a CSA8000 or TDS8000 instrument or its sampling modules.

#### **Compensation Requirement**

You must run a compensation (accessed from the Utilities menu) whenever the extender configuration is changed from that present at the last compensation. In short, if you install or remove an 80E00 extender, run a compensation. If you exchange a extender for one of a different length, run a compensation. For instructions on running a compensation, see the *CSA8000 and TDS8000 User Manual*.

### **Operating Temperature Requirement**

When you install one or more of the two-meter extenders, the operating temperature range of the instrument is reduced from +10 to +40 degrees C to +10 to +35 degrees C. The one-meter extender does not reduce the operating temperature range.

#### **Horizontal Position**

Inserting a sampling-module extender increases the minimum horizontal position settable by the instrument as follows:

- 1 meter: +5 ns
- 2 meter: +10 ns

**NOTE**. Because horizontal position is a global setting, installing an extender with any sampling module increases the minimum horizontal position setting for waveforms acquired from all modules, extended or not.

## **Installation Instructions**




**CAUTION.** To prevent damage to the sampling module or instrument, never install or remove this extender from the instrument or from the sampling module when the instrument is powered on. Observe standard handling precautions for static-sensitive devices while installing this kit. Always wear a grounded wrist strap, grounded foot strap, and static resistant apparel while installing this kit.

Also when installing or using this product, observe all static precautions and warnings listed in the User manuals for the sampling module and main instrument.

**NOTE**. The sampling-module extenders are keyed to prevent their connection to any device other than 80E00 Electrical Sampling Modules and to prevent two or more extenders from being connected in series.

Perform the following steps to install the extender between the instrument and the electrical sampling module:

- 1. If the instrument is running, shut it down by pressing the On/Standby button on the front panel.
- **2.** Install the connector labeled "To Instrument" into a suitable compartment in the instrument. See the sampling-module user manual if you require more information.

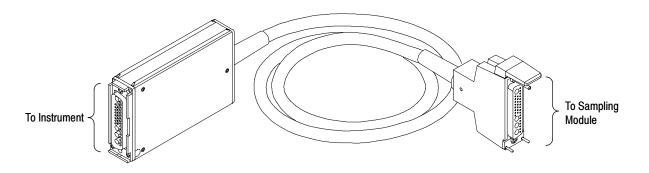

**3.** Use the connector marked "To Sampling Module" to connect to the sampling module. See the sampling-module user manual if you require information on connecting signals to the sampling module.

Installation Instructions